



KAHUNA BRACE

Instructions for Use


Kahuna Brace Fitting Instructions

The Kahuna Brace is universal and can be applied to the right or the left side of the patient. When properly applied, the Kahuna Brace can achieve various abduction angles from 30 to 90 degrees. When configured properly with the Airplane control bar, the Kahuna brace fits the description of the L3960 HCPC.

- Warning:** The Kahuna brace is supportive only and does not guarantee or intend to prevent injury. Consumer or patient agrees to the following.
- ManaMed accepts no responsibility for any injury which might occur while using ManaMed products.
 - Skin irritation may occur while using this device. If you experience an unusual skin reaction while using this product, consult with your healthcare provider immediately.
 - Consult your health care provider for this products indication for use.
 - For single patient use only.
 - Federal Law restricts this device to sale or by or on the order of a licensed health care practitioner.
 - If you do not agree to the above conditions, contact your health care provider before using this product.


- a. Kahuna Brace
- c. Ball

- b. Airplane Bar
- d. Distance

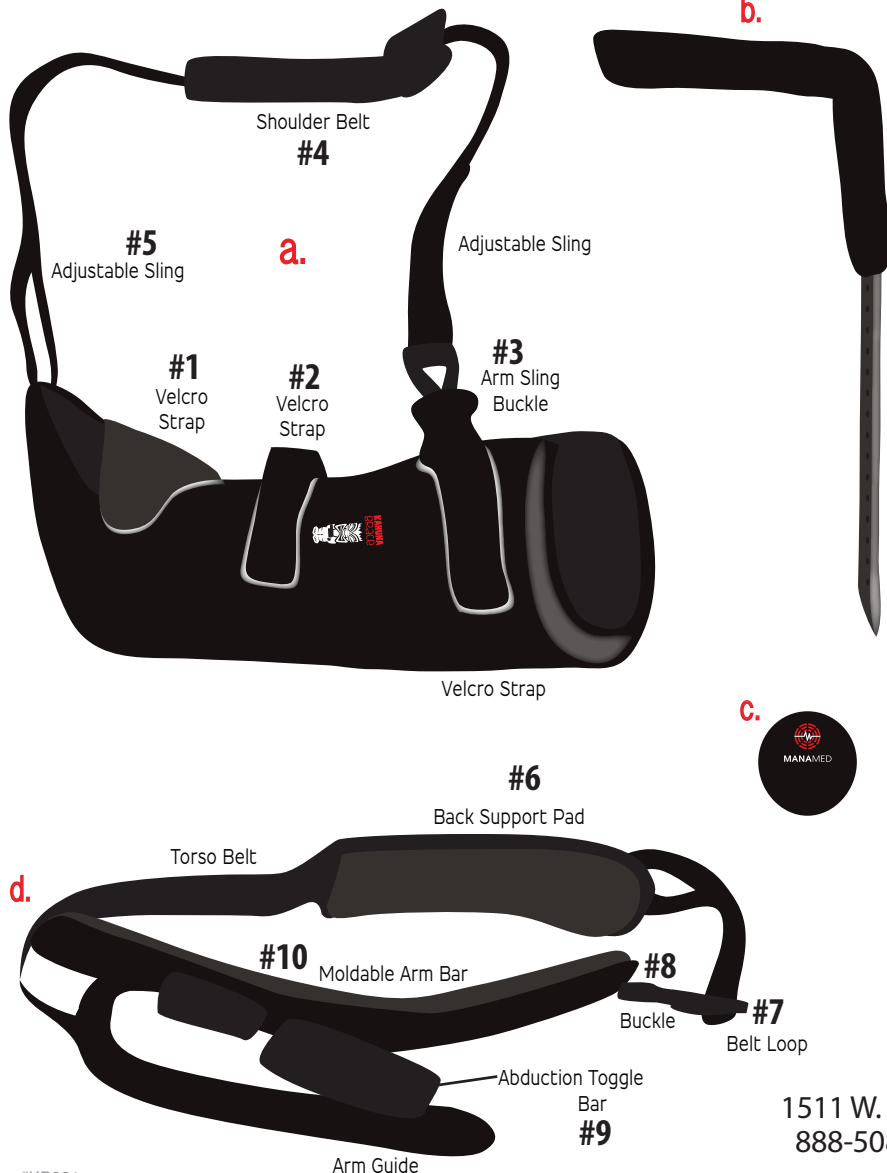

Application of the Kahuna Brace:


1. Open Velcro strap #1 and #2, also open buckle on the arm sling buckle #3. Place arm in the brace and secure both Velcro strap #1 & #2 comfortably around arm. To fit your arm into the sling you can fold the sling along the pre folded point under the arm sling buckle #3.




Washing and Care:

The Kahuna brace may be cleaned by hand using a mild soap and warm water. Hang to dry. Do not place in washing machine or dryer.


2. Place shoulder belt #4 around the opposite shoulder and adjust the sling #5 to fit comfortably around the shoulder.




3. Position the back support pad #6 in the middle of the patients back. Then adjust the Torso strap by adjusting the belt loop #7 which is at the base of the buckle #8.




4. Position the abduction toggle bar #9 on the injured side of the body and position the moldable arm bar #10 should be pointed forward.



5. Adjust the abduction toggle bar #9 and the moldable arm bar #10 to desired position. Increasing abduction by pulling the abduction toggle bar #9 towards the body.



6. To adjust the Kahuna brace into Airplane position, attach the Airplane control bar remove the foam padding at the back of the moldable arm band #10 and there are 2 holes to insert the Airplane control bar. Insert 2 screws (provided with Allen wrench)



1511 W. Alton Ave., Santa Ana CA 92704
888-508-0712 • www.ManaMed.Net



MANAMED™